

A loading B
Unloading C
Strain


F16. 1


AL SY

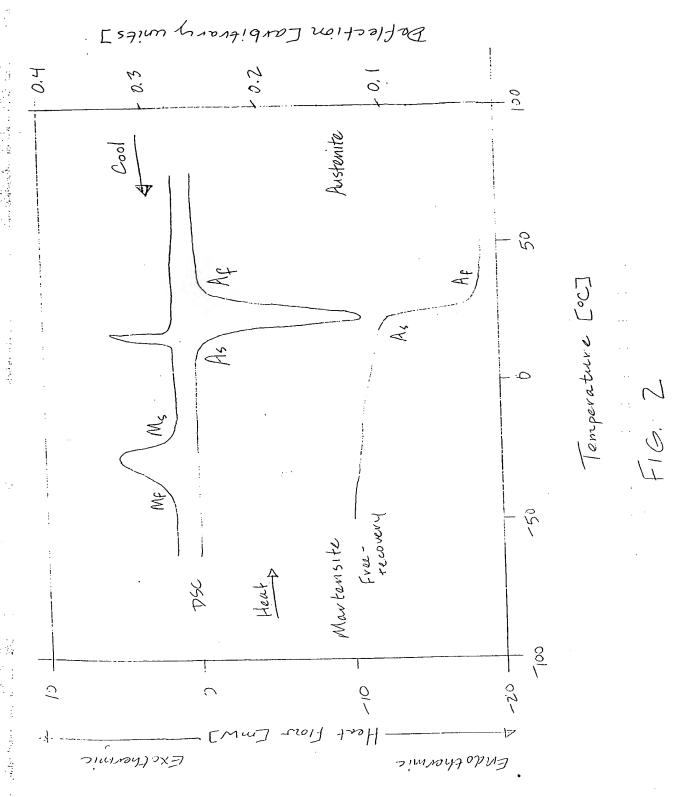

AVOIDING STRESS-INDUCED MARTENSITIC TRANSFORMATION IN MEDICAL DEVICES
SERIAL NO.: TBD; ENDOV-55675
SERIAL NO.: TBD; ENDOV-55675
SERIAL NO.: TBD; ENDOV-55675

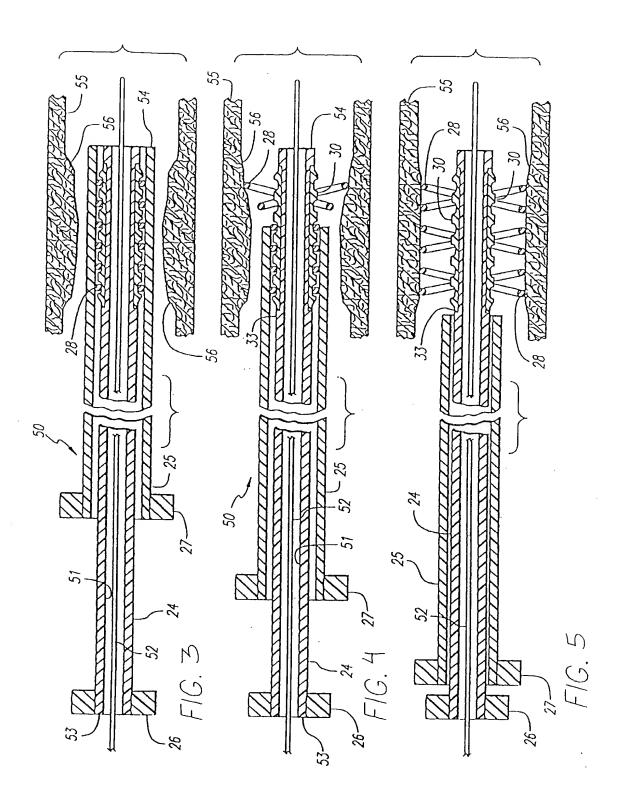

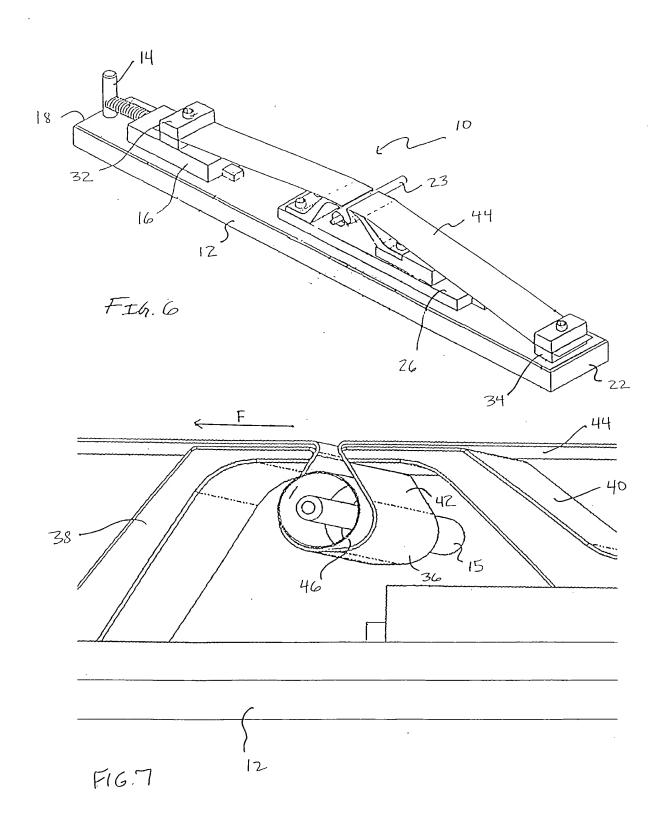

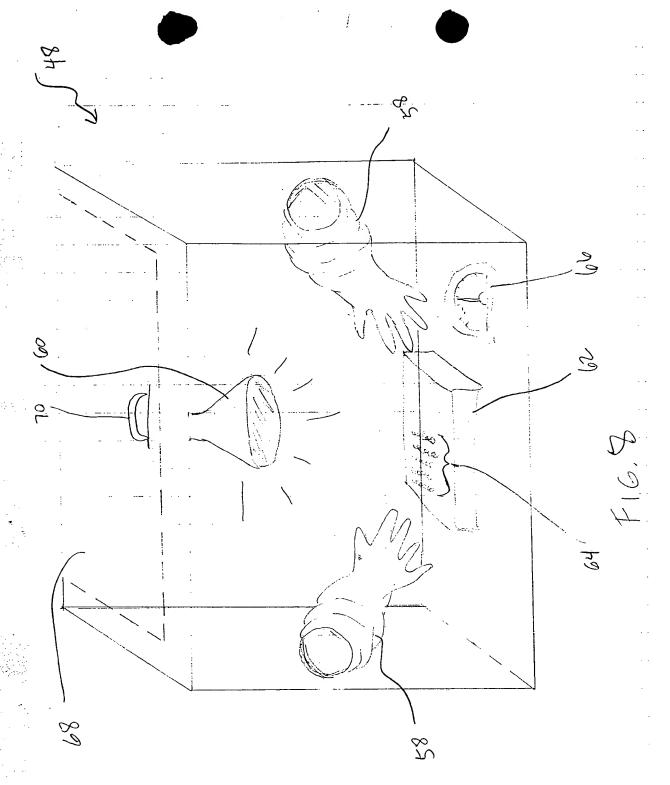

AVOIDING STRESS-INDUCED MARTENSITIC TRANSFORMATION IN SERIAL NO.: TBD; ENDOV-55675

SERIAL NO.: TBD; ENDOV-55675

